

# REPLACEMENT SHEET

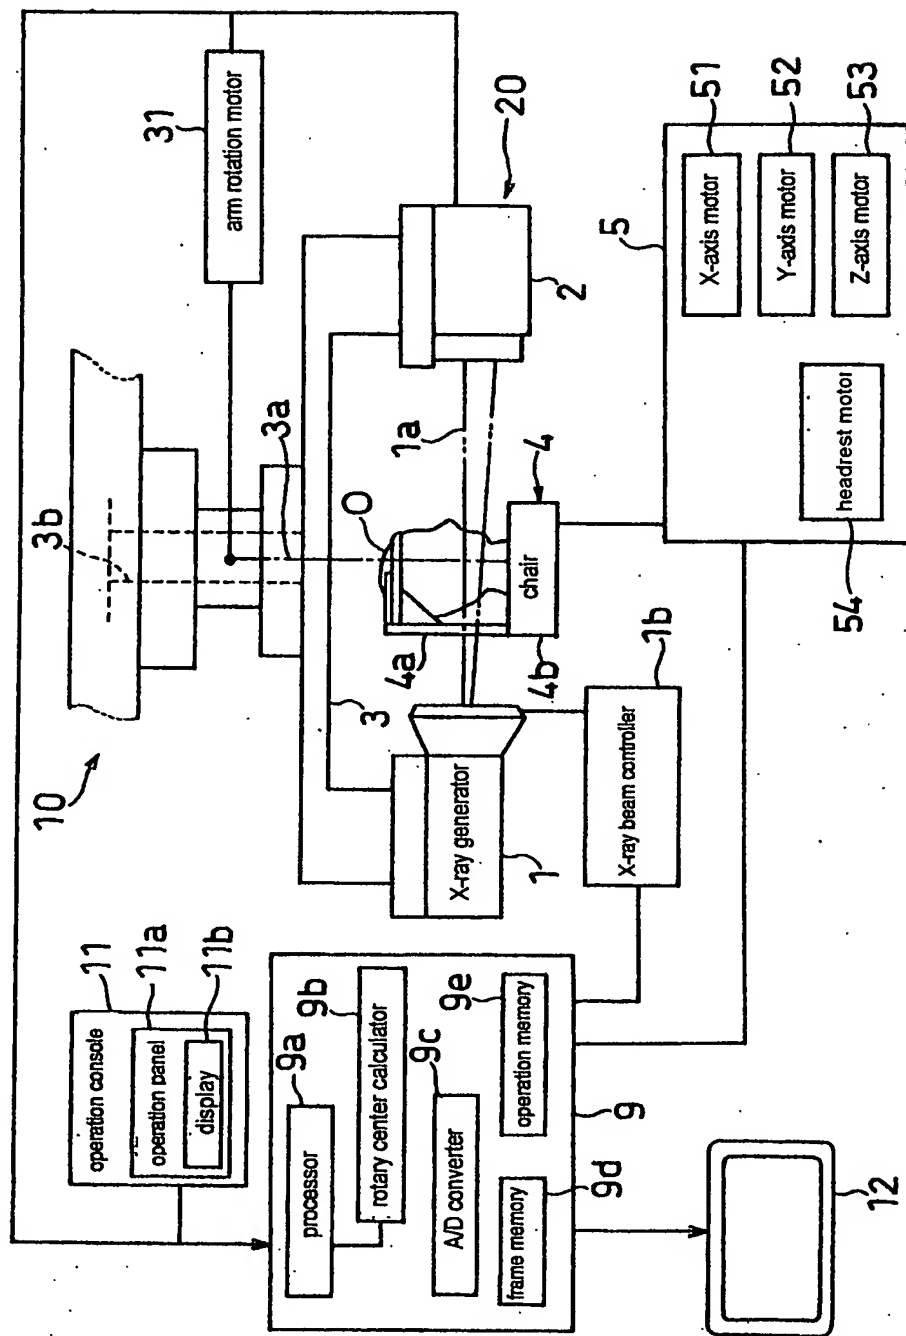
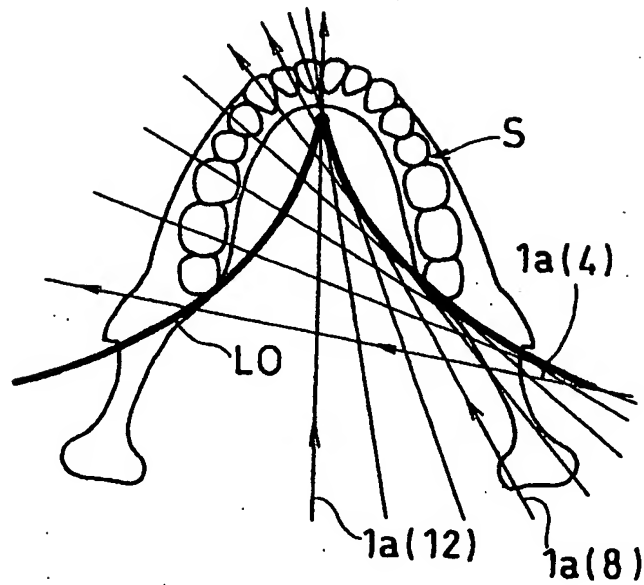
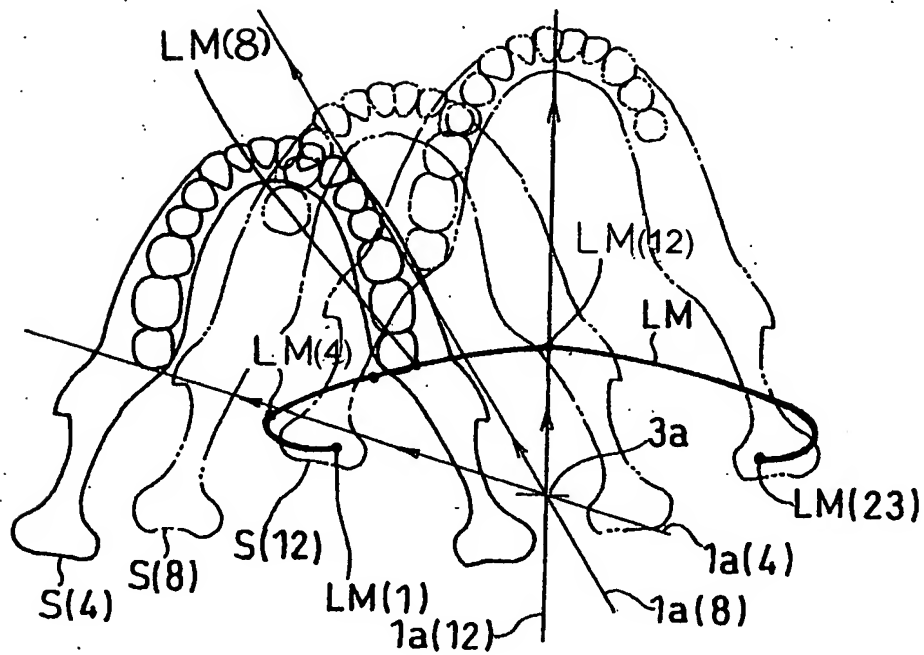


Fig.1

# REPLACEMENT SHEET



**Fig. 2 a**



**Fig. 2 b**

# REPLACEMENT SHEET

[ CT ] 0. 0 sec  
 projection method [ 360 degree projection ] 180 degree projection  
 copper filter [ 0. 25mm 0. 5mm 1. 0mm ]  
 patient size [ M ]  
 imaging area [ dental arch ]  
 80KV  
 4.0mA  
 slice angle [ 0 °c ]  
 Lock

\* 11b 11c

Fig.4

# REPLACEMENT SHEET

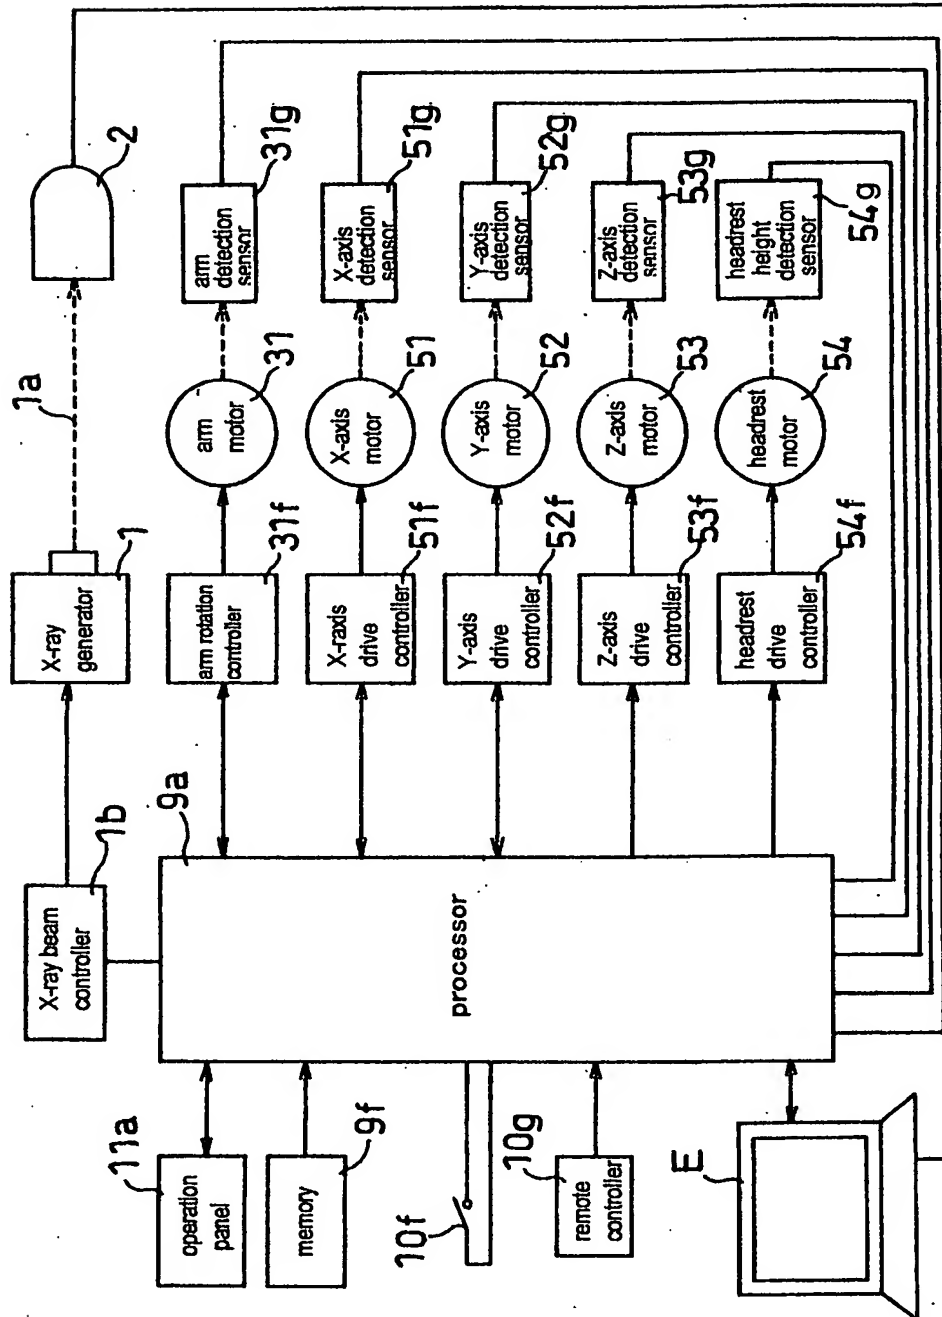
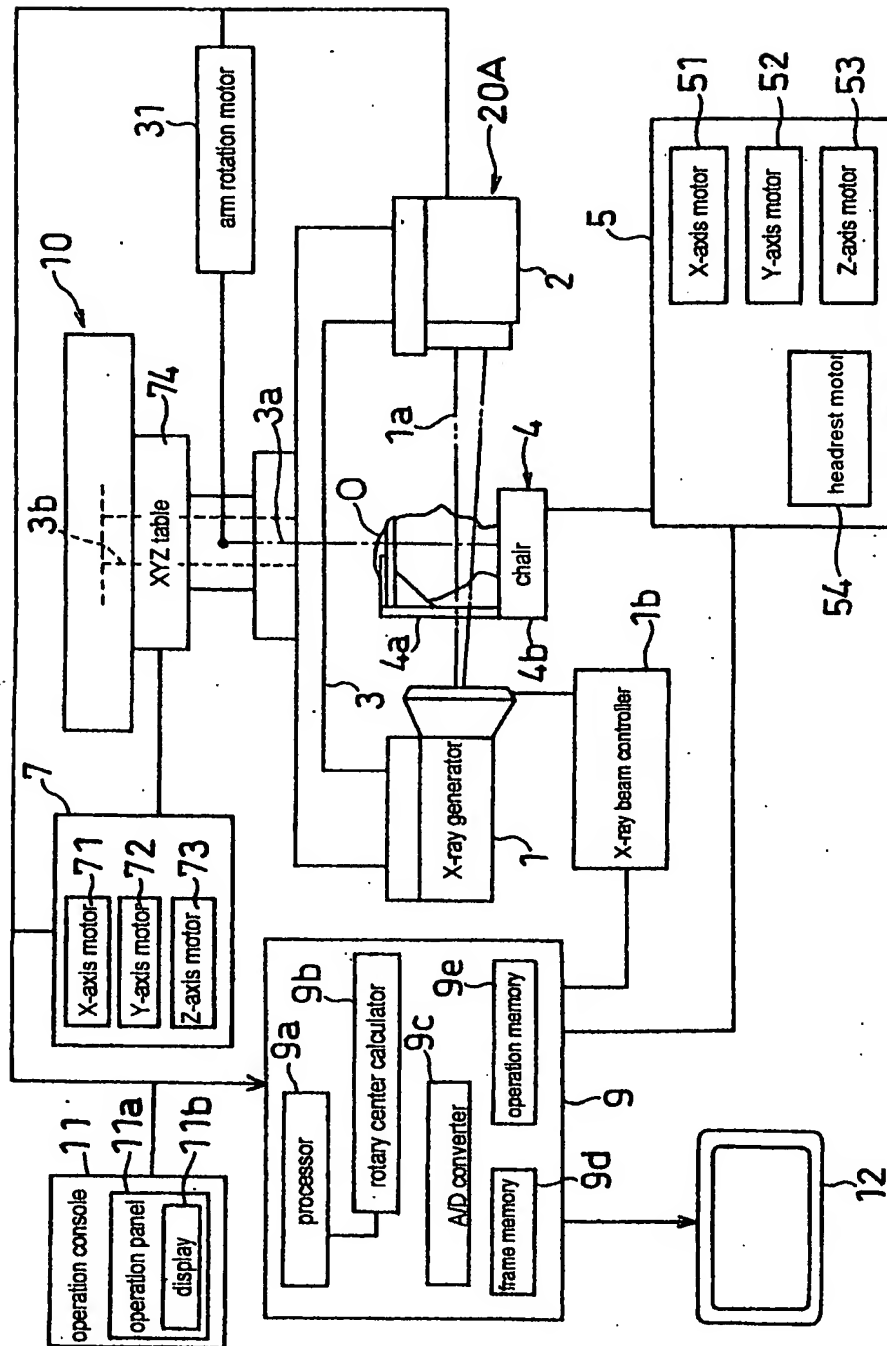


Fig. 9

# REPLACEMENT SHEET



**Fig. 14**

**Fig. 15**